

# Nitrogen Dioxide - Low Concentration

SENSOR ID: NO2\_LTSP1

Equipment ID: SL521251

Equip. Name: NW Scential




Future of Sensory Technology



Report Date: 01.01.2022 - 01.31.2022

Last Calibration: 03.04.2022

Report Generated: 03.08.2022

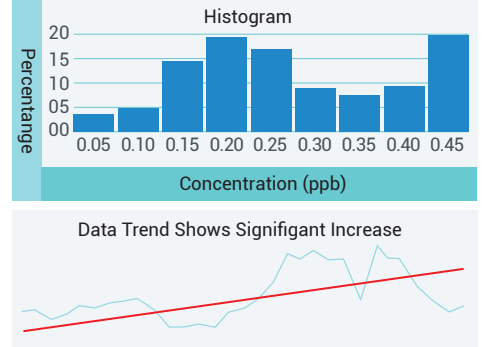

## AQ Box Graph

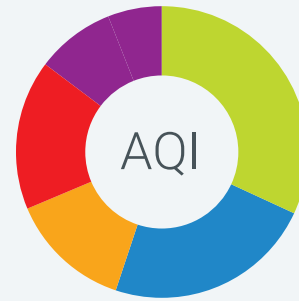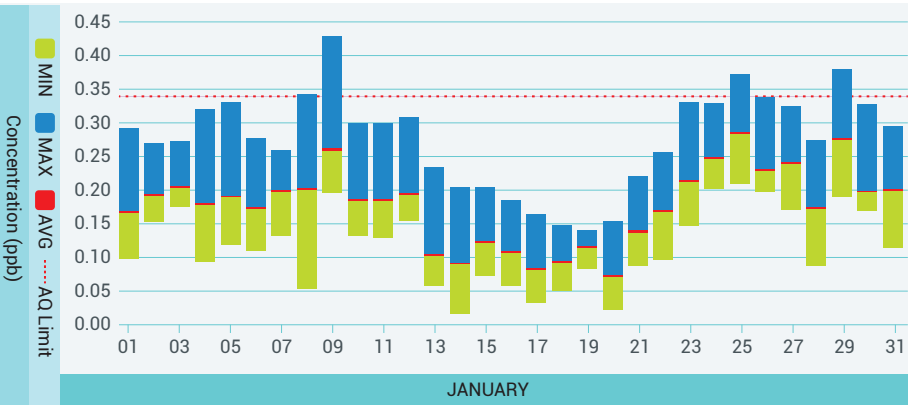

Exceedances

23

Exceeded Time

24%

Alarm Triggers

71

● moderate ● sensitive ● unhealthy  
● very unhealthy ● hazardous

AQI SETTINGS, AVG Period: Daily

Moderate: 50


Sensitive: 100

Unhealthy: 150

Very Unhealthy: 200

Hazardous: 250

## Heat Map

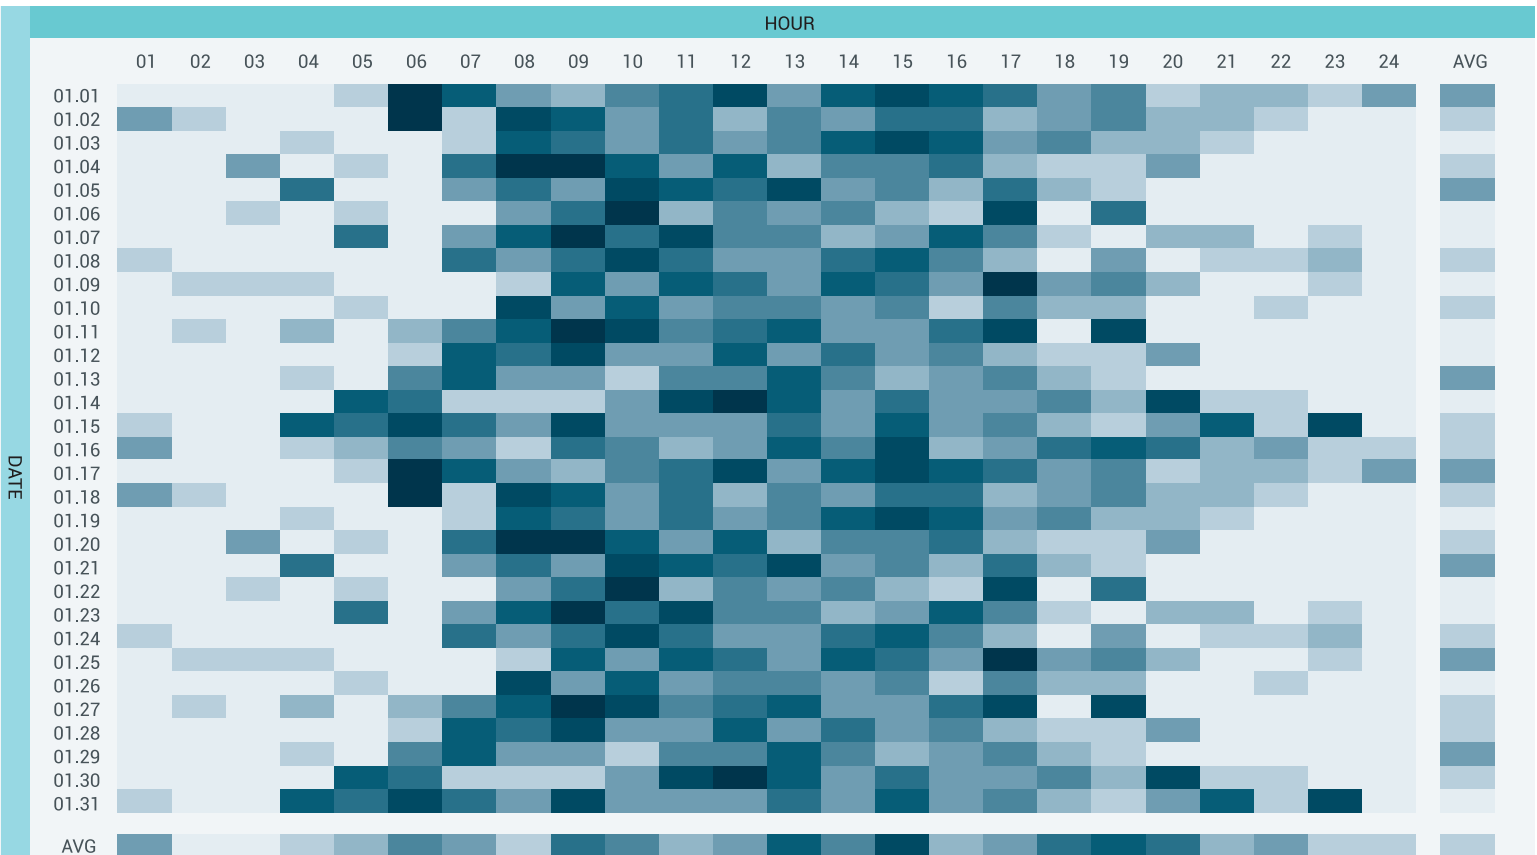

LEGEND (ppb) 0-0.2 0.2-0.4 0.4-0.6 0.6-0.8 0.8-1.0 1.0-1.2 1.2-1.4 1.4-1.6 1.6-1.8 1.8-2.0